


## Force Scientific Technologies Pvt. Ltd.

### ANALYTICAL DEVELOPMENT LABORATORY

<b>Sequence Directory :-</b>	UHPLC3\Method Development\Diclofenac IP Tablet.seq		
<b>Sequence Name :-</b>	Diclofenac IP Tablet	<b>Instrument ID :-</b>	UHPLC3
<b>Injection Name :-</b>	Diclofenac IP Tablet	<b>Column No. :-</b>	n.a.
<b>Injection No. :-</b>	10	<b>Vial Position :-</b>	Y:F2
<b>Injection Type :-</b>	Check Standard	<b>Injection Volume :-</b>	20.0 µL
<b>Instrument Method :-</b>	Diclofenac IP Tablet	<b>Run Time :-</b>	50.0 mins
<b>Processing Method :-</b>	3D Quantitative	<b>Analyst :-</b>	adl
<b>Injection Acquired On :-</b>	01.04.2024 22:40:54	<b>Wavelength :-</b>	254 nm

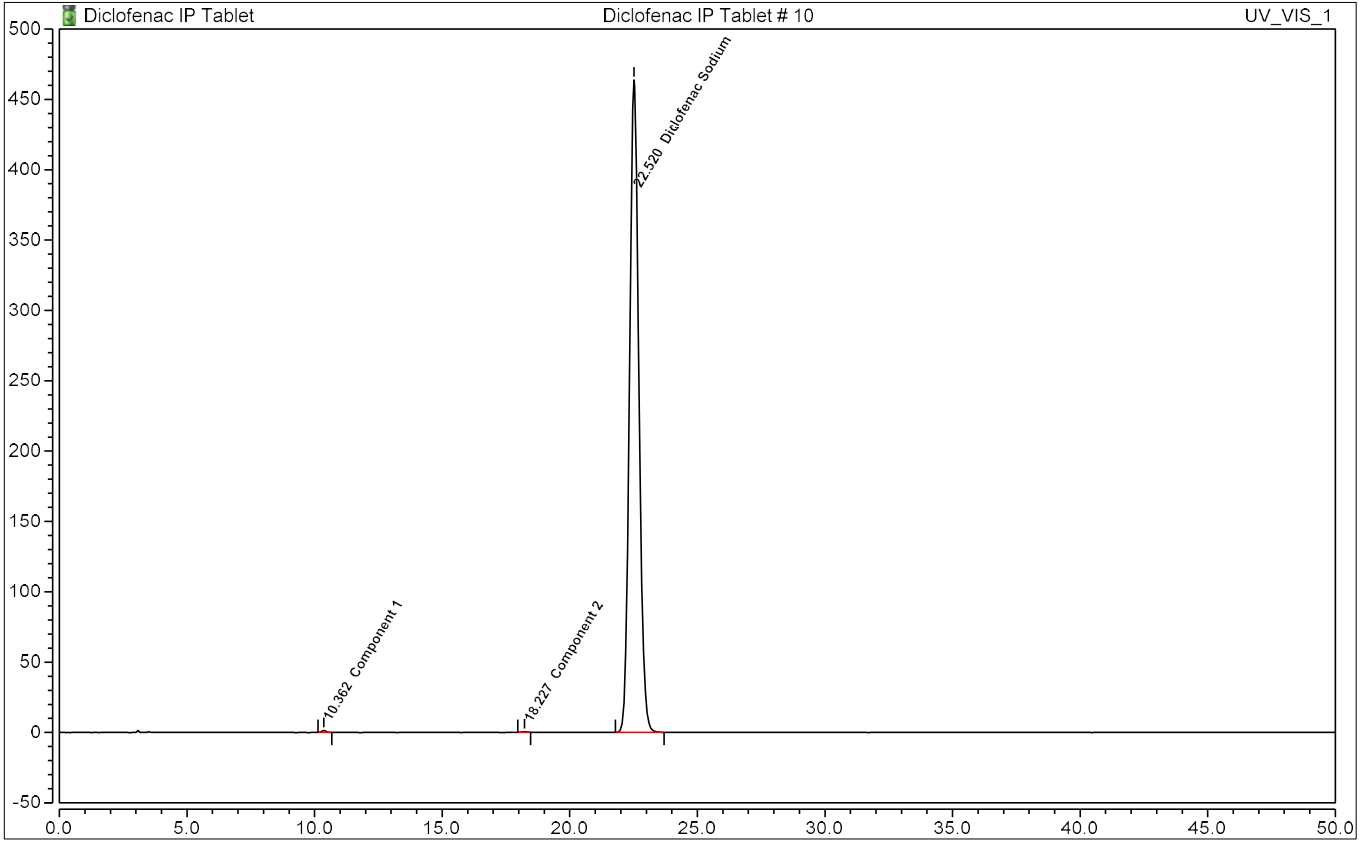


Peak No.	Ret. Time min	Peak Name	Area µAU*sec	Area %	Tailing (USP)	Resolution (USP)	Theoretical Plates	t. Time. (Diclofenac S)
1	10.362	Component 1	17464	0.15	1.09	n.a.	15633	0.46
2	18.227	Component 2	7112	0.06	0.95	20.07	25979	0.81
3	22.520	Diclofenac Sodium	11764388	99.79	1.09	7.67	18233	1.00
<b>Total</b>			<b>11788963</b>	<b>100.00</b>				

## Force Scientific Technologies Pvt. Ltd.

### ANALYTICAL DEVELOPMENT LABORATORY

<b>Sequence Directory :-</b>	UHPLC3\Method Development\Diclofenac IP Tablet.seq		
<b>Sequence Name :-</b>	Diclofenac IP Tablet	<b>Instrument ID :-</b>	UHPLC3
<b>Injection Name :-</b>	Diclofenac IP Tablet	<b>Column No. :-</b>	n.a.
<b>Injection No. :-</b>	11	<b>Vial Position :-</b>	Y:F3
<b>Injection Type :-</b>	Unknown	<b>Injection Volume :-</b>	20.0 µL
<b>Instrument Method :-</b>	Diclofenac IP Tablet	<b>Run Time :-</b>	50.0 mins
<b>Processing Method :-</b>	3D Quantitative	<b>Analyst :-</b>	adl
<b>Injection Acquired On :-</b>	01.04.2024 23:32:09	<b>Wavelength :-</b>	254 nm

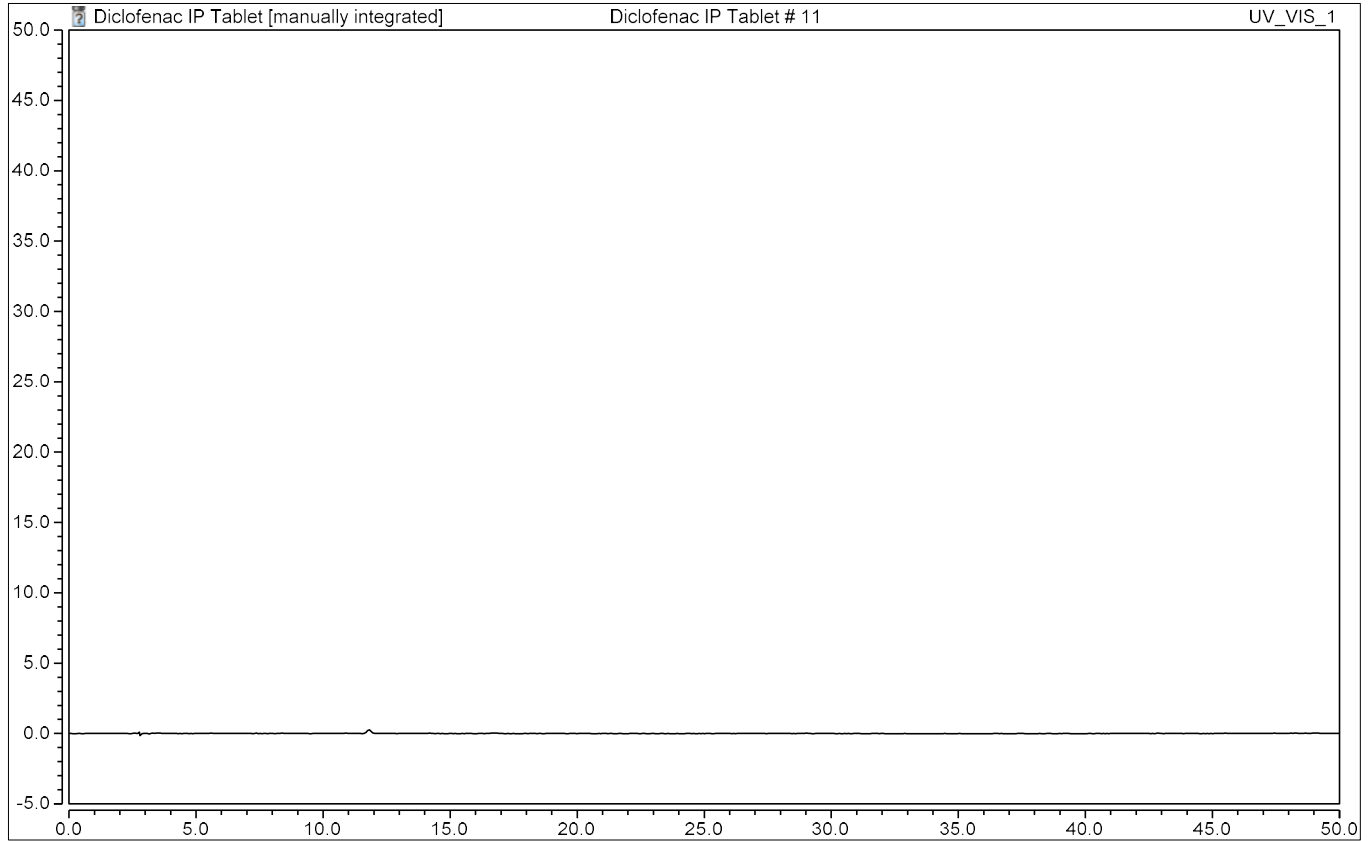


Peak No.	Ret. Time min	Peak Name	Area µAU*sec	Area %	Tailing (USP)	Resolution (USP)	Theoretical Plates	RRT
<b>Total</b>			<b>0</b>	<b>0.00</b>				

## Force Scientific Technologies Pvt. Ltd.

### ANALYTICAL DEVELOPMENT LABORATORY

<b>Sequence Directory :-</b>	UHPLC3\Method Development\Diclofenac IP Tablet.seq		
<b>Sequence Name :-</b>	Diclofenac IP Tablet	<b>Instrument ID :-</b>	UHPLC3
<b>Injection Name :-</b>	Diclofenac IP Tablet	<b>Column No. :-</b>	n.a.
<b>Injection No. :-</b>	10	<b>Vial Position :-</b>	Y:F2
<b>Injection Type :-</b>	Check Standard	<b>Injection Volume :-</b>	20.0 µL
<b>Instrument Method :-</b>	Diclofenac IP Tablet	<b>Run Time :-</b>	50.0 mins
<b>Processing Method :-</b>	3D Quantitative	<b>Analyst :-</b>	adl
<b>Injection Acquired On :-</b>	01.04.2024 22:40:54	<b>Wavelength :-</b>	254 nm

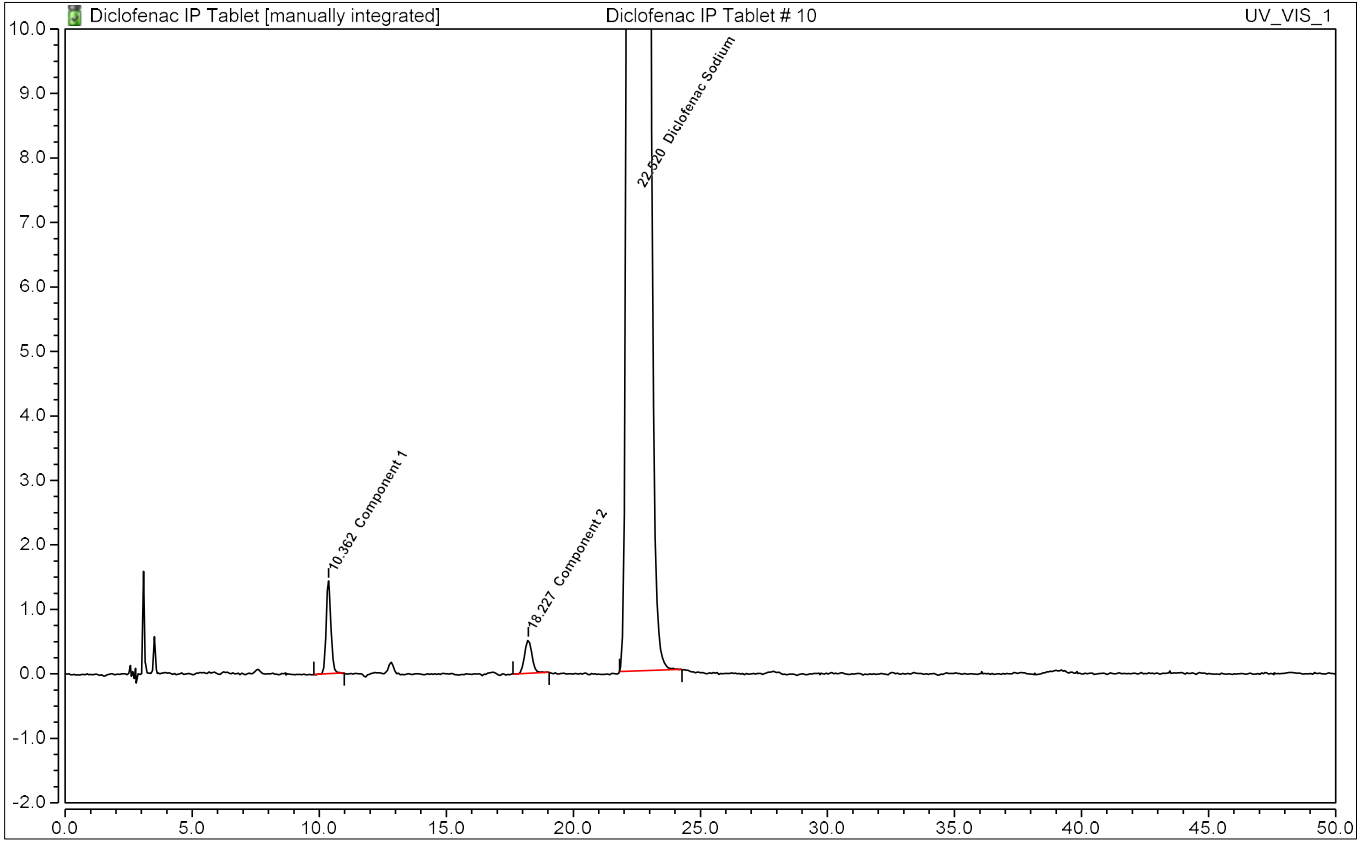


Peak No.	Ret.Time min	Peak Name	Area µAU*sec	Area %	Tailing (USP)	Resolution (USP)	Theoretical Plates	Ret.Time. (Diclofenac S
1	10.362	Component 1	18329	0.16	1.11	n.a.	15270	0.46
2	18.227	Component 2	10362	0.09	1.06	16.95	15138	0.81
3	22.520	Diclofenac Sodium	11766622	99.76	1.09	6.82	18233	1.00
<b>Total</b>			<b>11795313</b>	<b>100.00</b>				

## Force Scientific Technologies Pvt. Ltd.

### ANALYTICAL DEVELOPMENT LABORATORY

<b>Sequence Directory :-</b>	UHPLC3\Method Development\Diclofenac IP Tablet.seq		
<b>Sequence Name :-</b>	Diclofenac IP Tablet	<b>Instrument ID :-</b>	UHPLC3
<b>Injection Name :-</b>	Diclofenac IP Tablet	<b>Column No. :-</b>	n.a.
<b>Injection No. :-</b>	10	<b>Vial Position :-</b>	Y:F2
<b>Injection Type :-</b>	Check Standard	<b>Injection Volume :-</b>	20.0 µL
<b>Instrument Method :-</b>	Diclofenac IP Tablet	<b>Run Time :-</b>	50.0 mins
<b>Processing Method :-</b>	3D Quantitative	<b>Analyst :-</b>	adl
<b>Injection Acquired On :-</b>	01.04.2024 22:40:54	<b>Wavelength :-</b>	254 nm

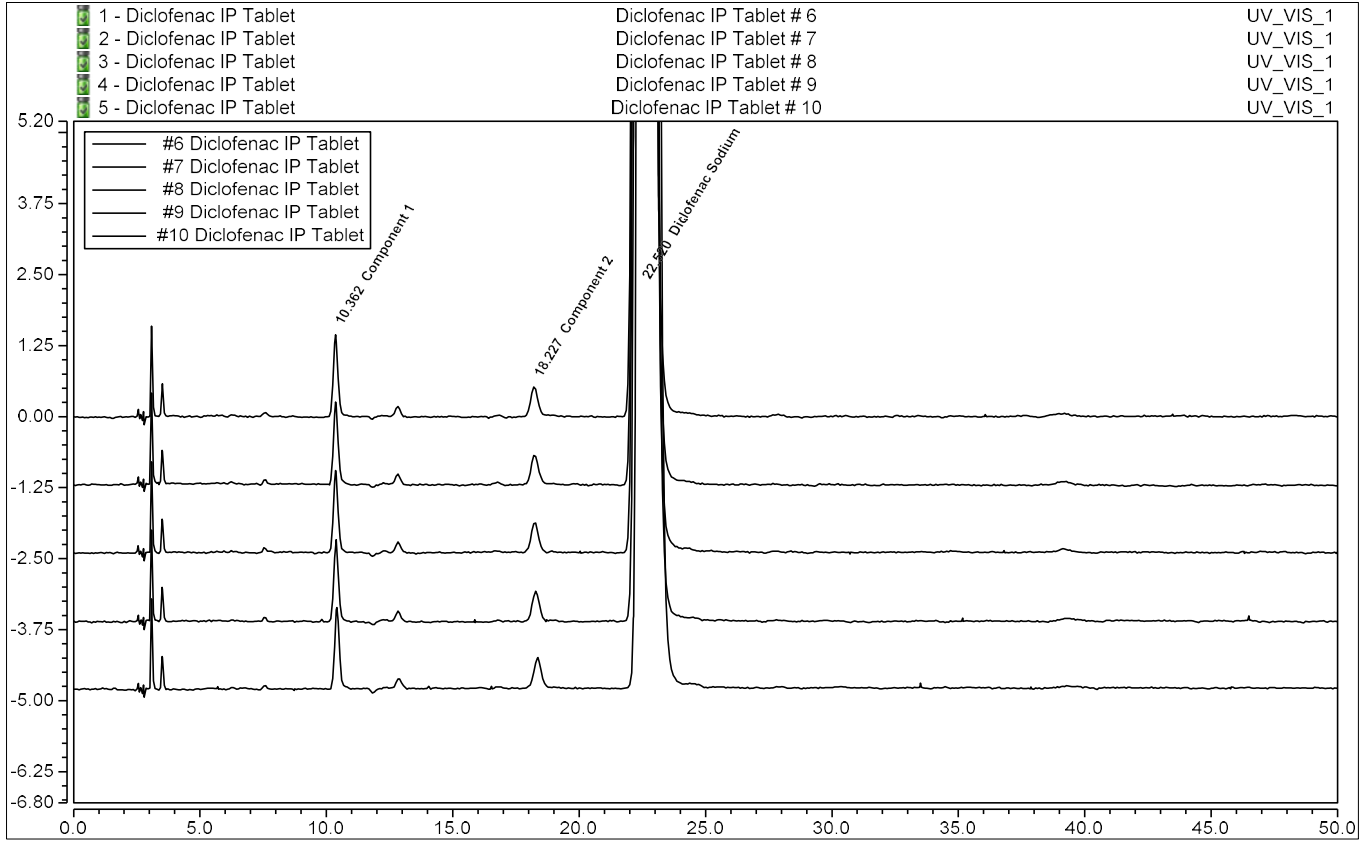

Peak No.	Ret.Time min	Peak Name	Area µAU*sec	Area %	Tailing (USP)	Resolution (USP)	Theoretical Plates	t.Time. (Diclofenac S
1	10.362	Component 1	17464	0.15	1.09	n.a.	15633	0.46
2	18.227	Component 2	7112	0.06	0.95	20.07	25979	0.81
3	22.520	Diclofenac Sodium	11764388	99.79	1.09	7.67	18233	1.00
<b>Total</b>			<b>11788963</b>	<b>100.00</b>				